

Supplemental Figure 1 – Ebola Treatment Center, Makeni Sierra Leone

Supplemental Figure 2 – The MultiSense™ patch

Supplemental Figure 3 – Components of the Modular Wireless Patient Monitoring System (MWPMS) transported in the pictured suitcase.

Supplemental Figure 4 - Total number of hours of data collected from each device used in the study (top), along with the % of data that passed an ECG signal quality test for data usability (bottom 2 graphs). The quality algorithm is based off of a higher order statistical analysis of the ECG signal calculated for every minute sample. The signal quality metric goes from 0 to 1, where 1 corresponds to a very high quality ECG signal and 0 corresponds to an unusable ECG signal. Any samples where the quality metric was below 0.75 were considered poor quality and removed from the data.

Supplemental Figure 5 – Screen shot of streamed continuous waveforms shown on the physIQ tablet app

Supplemental Figure 6 – Correlation between Medical team member-measured vital signs and near-simultaneous MultiSense patch measured value.


1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43

Supplemental Figure 1



<https://mc.manuscriptcentral.com/bmjgh>

Supplemental Figure 2

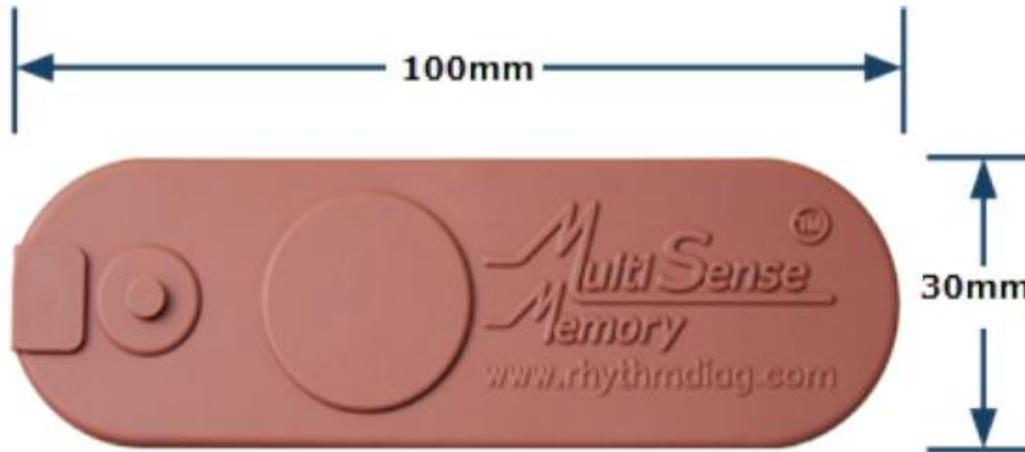


Supplemental Figure 3

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43



Supplemental Figure 4

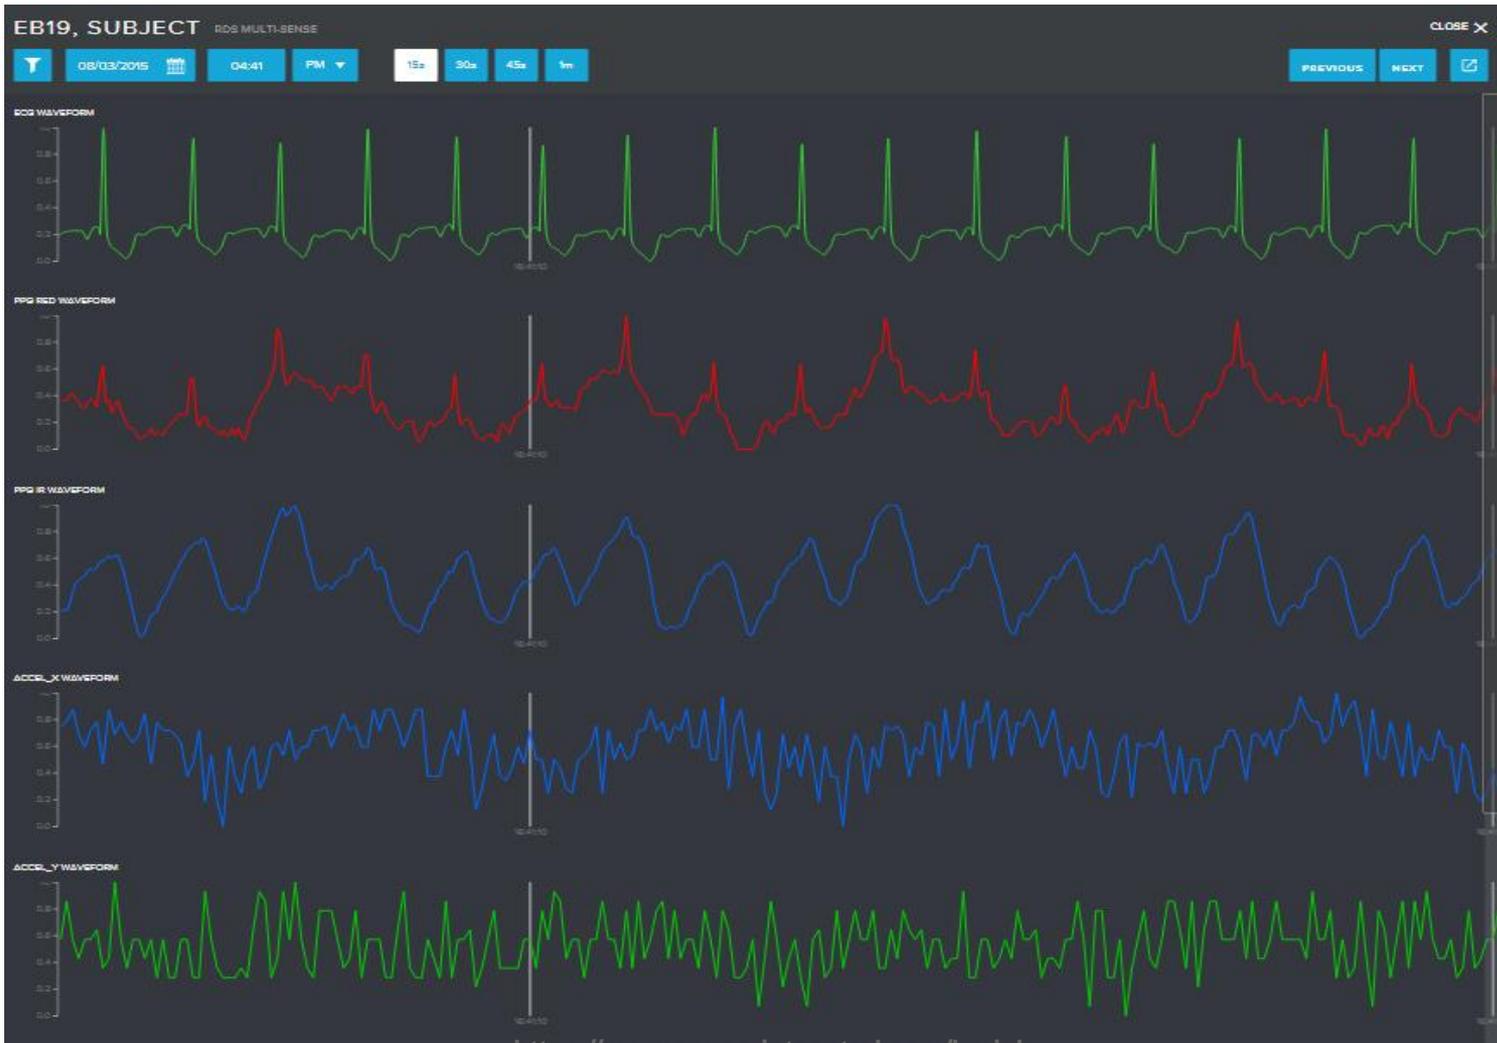

<https://mc.manuscriptcentral.com/bmjgh>

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43

Supplemental Figure 5

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43

